

Theoretical basis, application, reliability, and sample size estimates of a Meridian Energy Analysis Device for Traditional Chinese Medicine Research

Ming-Yen Tsai,^{1,*} Shih-Yu Chen,¹¹ Chung-Chun Lin¹

¹Department of Chinese Medicine, Kaohsiung Chang Gung Memorial Hospital and Chang Gung University College of Medicine, Kaohsiung, Taiwan.

¹¹School of Chinese Medicine for Post Baccalaureate, I-Shou University College of Medicine, Kaohsiung, Taiwan.

OBJECTIVES: The Meridian Energy Analysis Device is currently a popular tool in the scientific research of meridian electrophysiology. In this field, it is generally believed that measuring the electrical conductivity of meridians provides information about the balance of bioenergy or Qi-blood in the body.

METHODS AND RESULTS: PubMed database based on some original articles from 1956 to 2014 and the authors' clinical experience. In this short communication, we provide clinical examples of Meridian Energy Analysis Device application, especially in the field of traditional Chinese medicine, discuss the reliability of the measurements, and put the values obtained into context by considering items of considerable variability and by estimating sample size.

CONCLUSION: The Meridian Energy Analysis Device is making a valuable contribution to the diagnosis of Qi-blood dysfunction. It can be assessed from short-term and long-term meridian bioenergy recordings. It is one of the few methods that allow outpatient traditional Chinese medicine diagnosis, monitoring the progress, therapeutic effect and evaluation of patient prognosis. The holistic approaches underlying the practice of traditional Chinese medicine and new trends in modern medicine toward the use of objective instruments require in-depth knowledge of the mechanisms of meridian energy, and the Meridian Energy Analysis Device can feasibly be used for understanding and interpreting traditional Chinese medicine theory, especially in view of its expansion in Western countries.

KEYWORDS: Meridian Analysis; Electrical Conductance; Application; Traditional Chinese Medicine.

Tsai MY, Chen SY, Lin CC. Theoretical basis, application, reliability, and sample size estimates of a Meridian Energy Analysis Device for Traditional Chinese Medicine Research. *Clinics*. 2017;72(4):254-257

Received for publication on November 14, 2016; First review completed on December 26, 2016; Accepted for publication on February 14, 2017

*Corresponding author. E-mail: missuriae@yahoo.com.tw

Scientific publications utilizing Meridian Energy Analysis Devices (MEADs) as an index of meridian energy investigation are increasing in number year by year. It would therefore seem logical to conclude that the many researchers who publish scholarly articles using such devices are fully aware of their non-invasive nature and cost-effectiveness, two desirable qualities of any clinical measurement. Recent reviews of the literature demonstrate that no adequate consensus on either of these qualities has been fully reached (1,2).

According to MEAD Theory, developed by Dr. Yoshio Nakanani in the 1950s, the right and left side of the body respectively have 12 meridian lines. As shown in Figures 1A and 1B, MEAD can reflect the conditions of certain organs through analysis of the symmetrical Yuan points on the

wrists and ankles and comparison of their mutual relations and changes with micro-electrical currents to represent the physiological and pathological phenomena of the relevant meridians (3,4). The MEAD usually indicates constant values in the human body in the absence of external stimulation, visceral abnormalities, or diseases. The device is basically an amperometer employing a DC voltage of 12 V with output current of 0-200 μ A. An electrical current between two acupoints of larger than 90 μ A or smaller than 50 μ A represents an excess or deficiency syndrome in the meridian, respectively. The procedure of the MEAD is similar to equipment described in our previous study (5). The examination room should be bright, quiet, and refreshing, with a comfortable ambient temperature. The participants should refrain from engaging in physical activity, using tobacco, ingesting caffeine, or eating for at least one hour before clinical assessment. Before the assessment begins, they must remove all metal materials or body ornaments and lie flat to rest for 15 minutes. One metal cylinder is held in the left hand of the participant. The other, a spring-loaded probe, is moistened with 5% saline and, after sterilization, applied sequentially to the 24 Yuan acupoints: Lung (Taiyuan, LU9), Pericardium

Copyright © 2017 CLINICS – This is an Open Access article distributed under the terms of the Creative Commons License (<http://creativecommons.org/licenses/by/4.0/>) which permits unrestricted use, distribution, and reproduction in any medium or format, provided the original work is properly cited.

No potential conflict of interest was reported.

DOI: 10.6061/clinics/2017(04)10

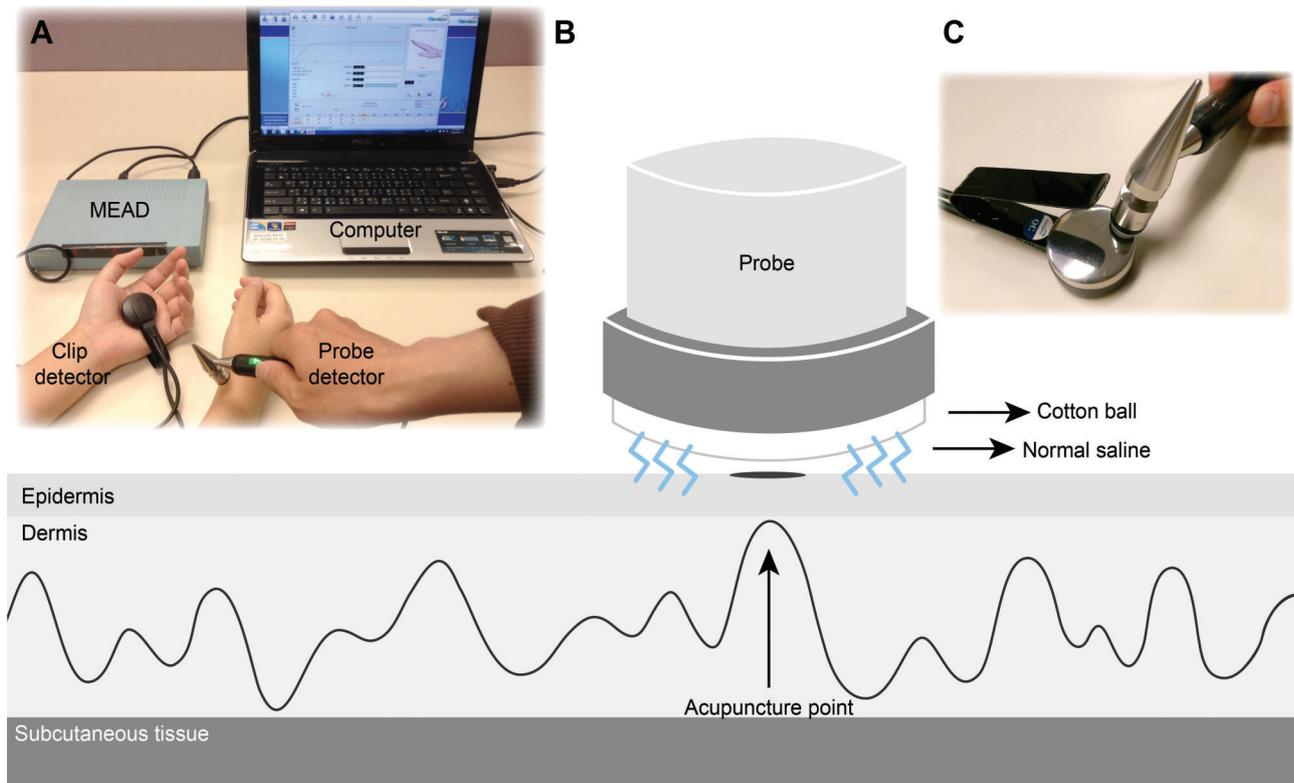


Figure 1 - Diagram of the schematic meridian energy analysis device (MEAD). Figures 1A and 1B: The experimental setup of the MEAD Instrument and electric current measurement around the acupoints. Figure 1C: A simple way to confirm the accuracy of MEAD using automatic digital calibration systems.

(Daling, PC7), Heart (Shenmen, HT7), Small Intestine (Wangu, SI4), Triple Energizer (Yangchi, TE4), Large Intestine (Hegu, LI5), Spleen (Taibai, SP3), Liver (Taichong, LR3), Kidney (Taixi, KI3), Urinary Bladder (Jinggu, BL65), Gallbladder (Qixu, GB40), and Stomach (Chongyang, ST42). (Figure 2) After 2-3 seconds of 12 g/cm² pressure for each point, the device is automatically interrupted, and the average value is recorded on a computerized system.

The application of MEAD is of high clinical interest not only in the objective assessment of traditional Chinese medicine (TCM) therapy and related sympathetic conditions but also in predicting the meridian flow of the corresponding organs. In 2012, Lin et al. used soft cupping with or without additional laser acupuncture and a MEAD for patients with low back pain (6). The results showed that pain scores were effectively alleviated after both treatments at the BL40. From observing the variations in the MEAD values of the Bladder Meridian, the authors concluded that soft cupping and laser acupuncture represent different purge and reinforcing characteristics in clinical practice. In a study by Hsu, healthy volunteers received short-term electrical acupuncture on the BL15, and the results revealed that a decrease in sympathetic activity after the intervention could be quantified with MEAD values (7). Another study showed that one measure of electrical conductance, the index of sympathovagal balance plus the calculus size in radiography, could be used as a valuable supplementary diagnostic method for selective urological intervention in patients with acute renal colic (8). In 2011, Huang et al. used a MEAD to detect the energy distribution of the meridian system after immediate glucose ingestion in different physical conditions (9). The findings suggested that

the glucose concentration in the blood was rapidly consumed and that the transformation in meridian energy was difficult to present in "Qi" vacuity groups after glucose intake. More recently, our own report also supported the verifiability of the promoting effect of coffee consumption on a specific meridian channel (5). In that study, however, the indexes of the meridians did not provide sufficient evidence for analysis of autonomic response.

When the sympathetic activity in the patient's body is high, increased intradermal acetylcholine stimulates the secretions of sweat glands, which in turn increases skin conductance and decreases resistance. In other words, the function of peripheral autonomic innervation can be indirectly evaluated by measuring the electrical conductivity of acupoints. However, many technical factors can influence skin electrical impedance, including the size of the electrode, its contact time, and the amount of pressure it places on the skin, as well as the accuracy of the acupoint location, the bias of the control environment and, importantly, the degree of skin moisture (10,11). The variability in measurement caused by these factors casts doubt on the reliability of the measurement of skin conductance. This doubt is the reason why few references citing the validity of devices for such measurement appear in academic textbooks or high-quality, refereed journals.

Regarding the electrical activity at acupoints, Colbert et al. (2) assessed the reliability of MEAD measurement in an unrestricted-designed investigation for any diagnostic or medical condition in patients. Their study provided much useful information for the reader to use in determining the value of MEAD results in terms of retest reliability. They also raised the

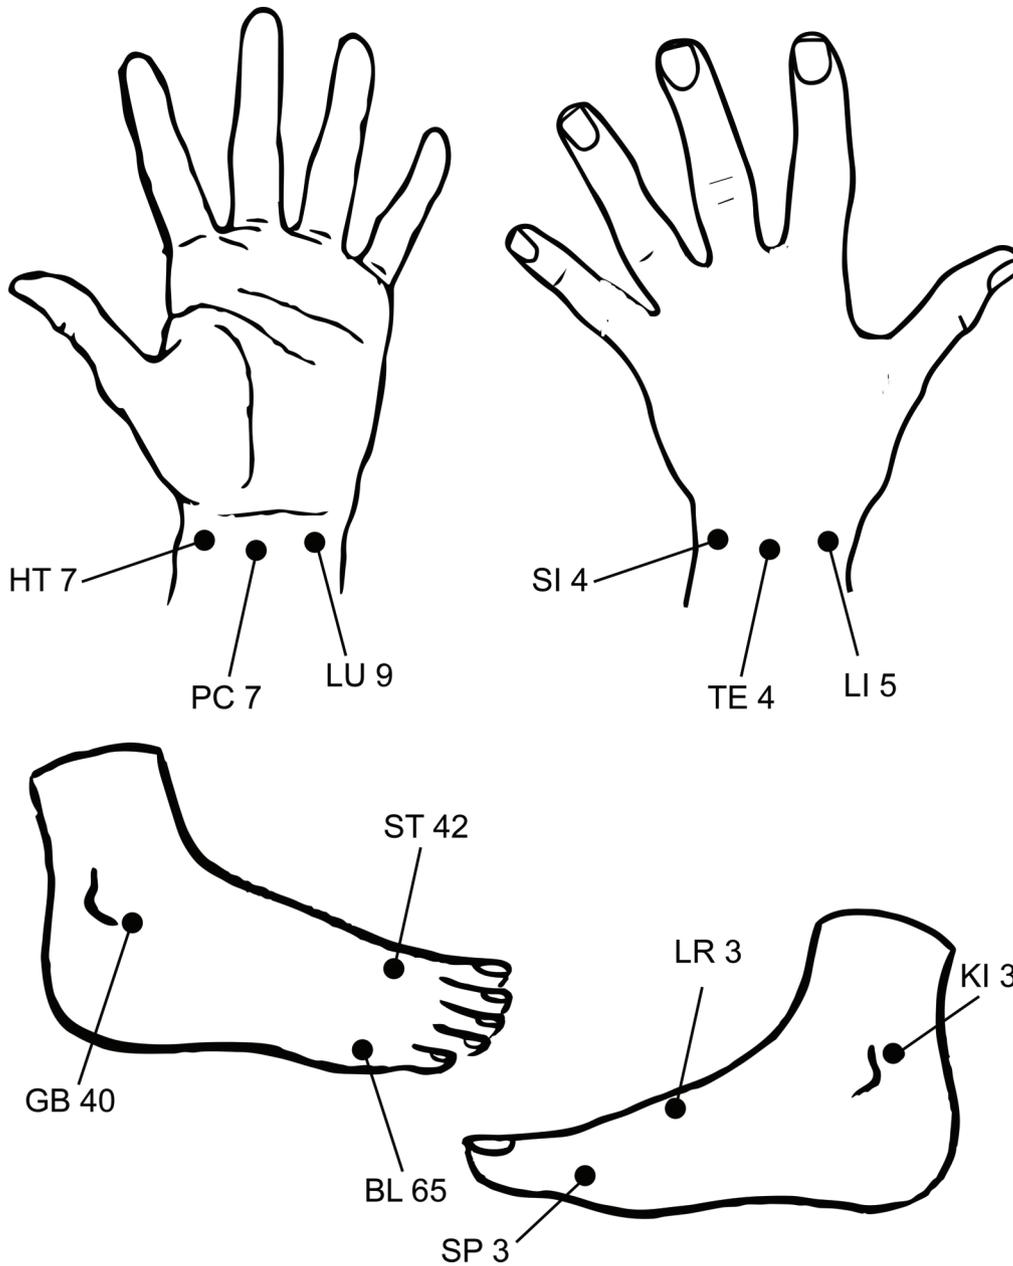


Figure 2 - The 24 MEAD measuring points on the hands and feet according to traditional Chinese medicine theory. (LU: Lung; PC Pericardium; HT: Heart; SI: Small Intestine; TE: Triple Energizer; LI: Large Intestine; SP: Spleen; LR: Liver; KI: Kidney; BL: Urinary Bladder; GB: gallbladder; ST: Stomach).

question of whether MEAD could be reliably used for diagnosis and/or therapeutic monitoring in the TCM field. The paper evaluates the reliability of selected studies and suggests a detailed procedure and methodology, as well as theoretical sample size requirements needed during future empirical investigations. A previous review (1) provided findings highly consistent with those of Colbert et al. Both studies concluded that the reliability of most electrical devices for the detection of meridian energy may appear low, or even unsatisfactory, for even the better-performing indices often double or halve the values from test to retest.

Although some studies quoted the earlier data of the device, the reproducibility is 93.2%, as reported by Nakatani (3), supporting the use of MEAD (12,13). Assessing the

reliability of MEAD in this way and the creation of blinding designs is challenging. To build consistency, skilled operators in possession of adequate information regarding the use of such instruments are necessary. However, the potential of subconscious bias from the operators may decrease the validity of MEAD measurement. For these reasons, proper preparation and steps are important to ensure consistent and reliable of MEAD measurement, as with any medical measurement device. In fact, experimental errors can be carefully controlled by operators, and the correlation coefficient can be used to confirm the stability of MEAD values (5,14). Newer MEAD machines also provide automatic digital calibration systems to help operators to exactly control the confounding factors. As shown in Figure 1C, when contacting the metal



clip with the probe produces electrical current up to 200 uA, it means that machine calibration is successful. MEAD is currently a convenient tool for TCM research, especially in the field of meridian electrophysiology.

To conclude, the assessment of TCM using objective modern instruments is just beginning. Many more rigorous studies are required in order to prove—or discredit—the value of MEAD measurement, which is largely ignored in the West. As illustrated in the article by Colbert et al. (2), such studies may also offer scientists well-reasoned items for both standardized methodology and design.

■ ACKNOWLEDGMENTS

This study was financially supported by the Chang Gung Memorial Hospital with grant number CMRPG 8F1391. The authors would like to thank Miss Hsiang-Yu Wang for figure drawing support.

■ AUTHOR CONTRIBUTIONS

All authors participated in the writing and discussed the final text.

■ REFERENCES

- Ahn AC, Colbert AP, Anderson BJ, Martinsen OG, Hammerschlag R, Cina S, et al. Electrical properties of acupuncture points and meridians: a systematic review. *Bioelectromagnetics*. 2008;29(4):245-56, <http://dx.doi.org/10.1002/bem.20403>.
- Colbert AP, Spaulding K, Larsen A, Ahn AC, Cutro JA. Electrodermal activity at acupoints: literature review and recommendations for reporting clinical trials. *J Acupunct Meridian Stud*. 2011;4(1):5-13, [http://dx.doi.org/10.1016/S2005-2901\(11\)60002-2](http://dx.doi.org/10.1016/S2005-2901(11)60002-2).
- Nakatani Y. Skin electric resistance and ryodoraku. *J Auton Nerv Syst*. 1956;6:52.
- Lee MS, Jeong SY, Lee YH, Jeong DM, Eo YG, Ko SB. Differences in electrical conduction properties between meridians and non-meridians. *Am J Chin Med*. 2005;33(5):723-8, <http://dx.doi.org/10.1142/S0192415X05003405>.
- Tsai MY, Kuo CE, Huang YC, Hsieh CL, Chen YH, Chen WC. Meridian energy analysis of the immediate effect of coffee consumption. *Eur J Integr Med*. 2014;6(1):74-81, <http://dx.doi.org/10.1016/j.eujim.2013.09.002>.
- Lin ML, Wu HC, Hsieh YH, Su CT, Shih YS, Lin CW, et al. Evaluation of the effect of laser acupuncture and cupping with ryodoraku and visual analog scale on low back pain. *Evid Based Complement Alternat Med*. 2012;2012:521612, <http://dx.doi.org/10.1155/2012/521612>.
- Hsu CC, Weng CS, Liu TS, Tsai YS, Chang YH. Effects of electrical acupuncture on acupoint BL15 evaluated in terms of heart rate variability, pulse rate variability and skin conductance response. *Am J Chin Med*. 2006;34(1):23-36, <http://dx.doi.org/10.1142/S0192415X06003606>.
- Lee CT, Chang YH, Lin WY, Xu JM, Chen HY, Chou PL, et al. Applications of meridian electrical conductance for renal colic: a prospective study. *J Altern Complement Med*. 2010;16(8):861-6, <http://dx.doi.org/10.1089/acm.2009.0273>.
- Huang KF, Tang ST, Chuang CY, Han WR, Lin JH, Young ST. Different patterns of dynamic variations on electrical conductances of acupoints between Qi Vacuity and Qi non-Vacuity after glucose ingestion. *J Altern Complement Med*. 2011;17(9):843-9, <http://dx.doi.org/10.1089/acm.2010.0528>.
- Evans WD, McClagish H, Trudgett C. Factors affecting the *in vivo* precision of bioelectrical impedance analysis. *Appl Radiat Isot*. 1998;49(5-6):485-7, [http://dx.doi.org/10.1016/S0969-8043\(97\)00061-4](http://dx.doi.org/10.1016/S0969-8043(97)00061-4).
- Ahn AC, Wu J, Badger GJ, Hammerschlag R, Langevin HM. Electrical impedance along connective tissue planes associated with acupuncture meridians. *BMC Complement Altern Med*. 2005;5:10, <http://dx.doi.org/10.1186/1472-6882-5-10>.
- Chien TJ, Liu CY, Lu RH, Kuo CW, Lin YC, Hsu CH. Therapeutic efficacy of traditional Chinese medicine, "Kuan-Sin-Yin", in patients undergoing chemotherapy for advanced colon cancer - a controlled trial. *Complement Ther Med*. 2016;29:204-12, <http://dx.doi.org/10.1016/j.ctim.2016.10.001>.
- Chien TJ, Liu CY, Ko PH, Hsu CH. A Chinese decoction, Kuan-Sin-Yin, improves autonomic function and cancer-related symptoms of metastatic colon cancer. *Integr Cancer Ther*. 2016;15(1):113-23, <http://dx.doi.org/10.1177/1534735415617282>.
- Chen CW, Tai CJ, Choy CS, Hsu CY, Lin SL, Chan WP, et al. Wave-induced flow in meridians demonstrated using photoluminescent bioceramic material on acupuncture points. *Evid Based Complement Alternat Med*. 2013;2013:739293, <http://dx.doi.org/10.1155/2013/739293>.